


Test Start Date/Time : XXXXXXXXXX
Filter ID : PLEATED_PTFE_CD7
Test Method : Bubble Point
Operator : XXXXXXXXXX
Filter Name : Pleated PTFE 10" Cartridge
Filter Type : 0.2 Hydrophobic
Batch No. : NA
Lot No. : T18012025-078
Filter Cat No. : 078
Test Location : XXXXXXXXXX
Test Gas : N₂
Wetting Fluid : 60.0 IPA / 40.0 WATER
Min. BPT Pressure : 1309.31 mbar
Max. BPT Pressure : 2068.43 mbar

Result : **PASS**

Measured BP : 1740.75 mbar
Test Duration : 5 min 44 sec
Test End Date/Time : 28/07/2025 11:38:54

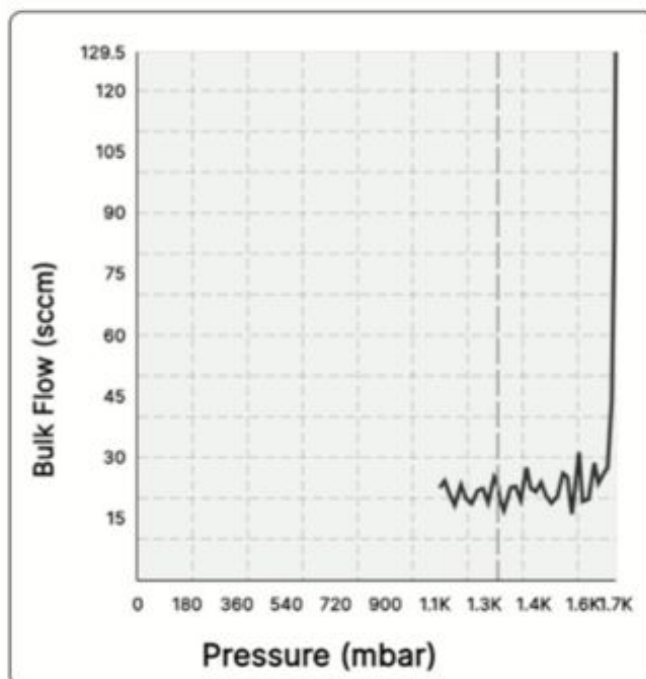

Notes

The following procedure is based on ASTM F316
(Standard Test Method for Bubble Point Test).